LIST OF PRODUCTS

* Digital Multimeter
* AC Clamp Adaptor
* Thermo Anemometer
* Distance Meter
* Network Cable Tester
* Earth Resistance Tester
* DC Power Supplies
* Calibrators
* Frequency Counter
* Phasing Sticks
* Waterproof Pen Testers
* EMF Detector
* Digital AC & AC/DC Clampmeter
* AC/DC Current Adaptor
* Thermo Hygrometer
* Digital Lux Meter
* Power Factor Regulator
* Digital Panel Meters
* High Voltage Detector
* Gas Analysers
* Function Generator
* Battery Tester
* Solar Power Meter
* Wood, Paper & Grain Moisture Meter
* Transistorised Electronic Analog & Digital Insulation Resistance Testers(upto 10 KV)
* Digital Sound Level Meter & Sound Level Calibrator
* Digital contact & Non-contact Type Tachometer
* Digital Non-contact (infrared) Thermometer
* Maximum Demand Controller/Digital Power Meter
* Digital Hand Held Temperature Indicators

Email : sales@kusam-meco.co.in

Website : www.kusamelectrical.com

13/11/2018

KUSAM-MECO®

AN ISO 9001:2015 COMPANY

AC / DC TRMS Clamp-On Multimeter with VFD, EF-Detection, PC Interface


MODEL - KM 2777

OPERATION MANUAL

KUSAM-MECO

AC / DC TRMS Clamp-On Multimeter with VFD, EF-Detection & PC Interface

MODEL - KM 2777

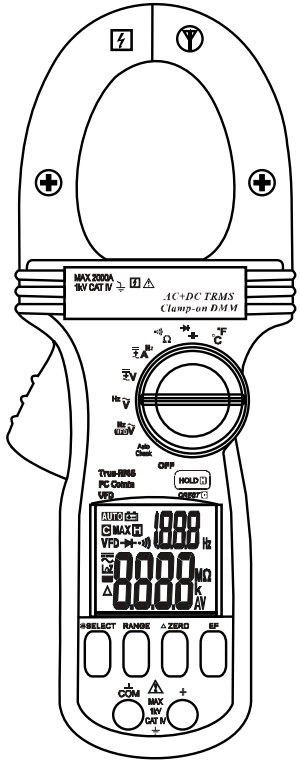

KUSAM-MECO

MUMBAI

TEST CERTIFICATE

This Test Certificate that warranty the product has been inspected and Tested in accordance with the published specifications. The instrument has been calibrated by using equipment which has already been calibrated to standards traceable to national standards.

MODEL NO. _____

SERIAL NO. _____

DATE: _____

ISO 9001:2015 REGISTERED

QC KUSAM-MECO PASS

WARRANTY

Each “KUSAM-MECO” product is warranted to be free from defects in material and workmanship under normal use & service. The warranty period is one year (12 months) and begins from the date of despatch of goods. In case any defect occurs in functioning of the instrument, under proper use, within the warranty period, the same will be rectified by us free of charges, provided the to and fro freight charges are borne by you. This warranty extends only to the original buyer or end-user customer of a “KUSAM-MECO” authorized dealer. This warranty does not apply for damaged Ic’s, fuses, disposable batteries, carrying case, test leads, or to any product which in “KUSAM-MECO’s” opinion, has been misused, altered, neglected, contaminated or damaged by accident or abnormal conditions of operation or handling. “KUSAM-MECO” authorized dealer shall extend this warranty on new and unused products to end-user customers only but have no authority to extend a greater or different warranty on behalf of “KUSAM-MECO”. “KUSAM-MECO’s” warranty obligation is limited, at option, free of charge repair, or replacement of a defective product which is returned to a “KUSAM-MECO” authorized service center within the warranty period.


blown off (become high impedance) like fuses to protect the user and the instrument. Most measuring functions through this terminal will then be open circuit.

Cleaning and Storage

Periodically wipe the case with a damp cloth and mild detergent; do not use abrasives or solvents. If the meter is not to be used for periods of longer than 60 days, remove the batteries and store them separately.

Battery Replacement

The meter uses standard 1.5V AA Size (IEC LR6) battery X 2
Loosen the 2 captive screws from the battery cover case. Lift the battery cover case. Replace the batteries. Replace battery cover case. Re-fasten the screws.

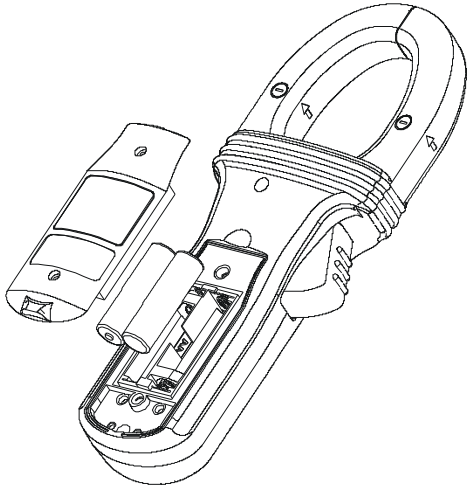

KUSAM-MECO

TABLE OF CONTENTS

TITLE	PAGE NO.
SAFETY	01
TERMS IN THIS MANUAL	02
INTERNATIONAL ELECTRICAL SYMBOL	03
FEATURES & GENERAL SPECIFICATION	04
ELECTRICAL SPECIFICATION	06
PRODUCT DESCRIPTION	14
OPERATION	15
MAINTENANCE	27
TEST CERTIFICATE	28
WARRANTY	29

1) SAFETY INFORMATION

This manual contains information and warnings that must be followed for operating the instrument safely and maintaining the instrument in a safe operating condition. If the instrument is used in a manner not specified by the manufacturer, the protection provided by the instrument may be impaired.

The meter protection rating, against the users, is double insulation per UL/IEC/EN61010-1 Ed. 3.0, IEC/EN61010-2-033 Ed. 1.0, CAN/CSA C22.2 No. 61010-1 Ed. 3.0, IEC/EN61010-2-032, Ed. 3.0 & IEC/EN61010-031 Ed. 1.1:

Measurement Category IV 1000V AC & DC.

Per IEC61010-1 OVERVOLTAGE CATEGORY

OVERVOLTAGE CATEGORY II (CAT II) is for equipment intended to be supplied from the building wiring. It applies both to plug-connected equipment and to PERMANENTLY CONNECTED EQUIPMENT.

OVERVOLTAGE CATEGORY III (CAT III) is for equipment intended to form part of a building wiring installation. Such equipment includes socket outlets, fuse panels, and some MAINS installation control equipment.

OVERVOLTAGE CATEGORY IV (CAT IV) is for equipment installed at or near the origin of the electrical supply to a building, between the building entrance and the main distribution board. Such equipment may include electricity tariff meters and primary overcurrent protection devices.

Auto-Power-Off (APO)

The Auto-Power-Off (APO) mode turns the meter off automatically to extend battery life after approximately 34 minutes of no rotary switch or push button operations. To wake up the meter from APO, press the **SELECT** button momentarily and release or turn the rotary switch OFF and then back on. Always turn the rotary switch to the OFF position when the meter is not in use.

Disabling Auto-Power-Off

Press and hold the **SELECT** button while turning the meter on to temporarily disable the Auto-Power-Off (APO) feature. Turn the rotary switch OFF and then back on to resume.

MAINTENANCE

WARNING

To avoid electrical shock, disconnect the meter from any circuit, remove the test leads from the input jacks and turn OFF the meter before opening the case. Do not operate with open case.

Trouble Shooting

If the instrument fails to operate, check batteries and test leads etc., and replace as necessary. Double check operating procedure as described in this user's manual.

If the instrument voltage-resistance input terminal has subjected to high voltage transient (caused by lightning or switching surge to the system under test) by accident or abnormal conditions of operation, the protective impedance components in series might be

Backlighted LCD display

Press the **SELECT** button for 1 second or more to toggle the LCD backlight. The backlight will also be turned off automatically after 32 seconds to extend battery life.

Relative-Zero (Δ) mode

Relative-Zero allows the user to offset the meter consecutive measurements with the main display displaying reading as the reference value. Press the **REL** button momentarily and release to toggle Relative-Zero mode.

Manual or Auto-ranging

Press the **RANGE** button momentarily and release to select manual-ranging, and the meter will remain in the range it was in, the LCD **AUTO** turns off. Press the button again to step through the ranges. Press and hold the button for 1 second or more and release to resume auto-ranging.

Note: manual-ranging feature is not available in **Hz** and ⊣⊢ function ranges.

Set Beeper Off

Press the **RANGE** button while turning the meter on to temporarily disable the Beeper feature. Turn the rotary switch OFF and then back on to resume.

TERMS IN THIS MANUAL

WARNING Identifies conditions and actions that could result in serious injury or even death to the user.

CAUTION Identifies conditions and actions that could cause damage or malfunction in the instrument.

WARNING

To reduce the risk of fire or electric shock, do not expose this product to rain or moisture. The meter is intended only for indoor use.

To avoid electrical shock hazard, observe the proper safety precautions when working with voltages above 60 VDC or 30VAC rms. These voltage levels pose a potential shock hazard to the user. Before & after hazardous voltage measurements, test the voltage function on a known source such as line voltage to determine proper meter functioning.

Keep your hands/fingers behind the hand/finger barriers (of the meter and the test leads) that indicate the limits of safe access of the hand-held part during measurement. Inspect test leads, connectors, and probes for damaged insulation or exposed metal before using the instrument. If any defects are found, replace them immediately. Only use the test lead provided with the equipment or UL Listed Probe Assembly rated CAT IV 1000V or better.

This Clamp-on meter is designed to apply around or remove from uninsulated hazardous live conductors. But still, individual protective equipment must be used if hazardous live parts in the installation where measurement is to be carried out could be accessible.

CAUTION Disconnect the test leads from the test points before changing meter functions.

INTERNATIONAL ELECTRICAL SYMBOLS

	Caution ! Refer to the explanation in this Manual
	Caution ! Risk of electric shock
	Earth (Ground)
	Double Insulation or Reinforced insulation
	Fuse
	AC--Alternating Current
	DC--Direct Current
	Application around and removal from hazardous live conductors is permitted

2) CENELEC Directives

The instruments conform to CENELEC Low-Voltage directive 2006/95/EC and Electromagnetic compatibility directive 2004/108/EC.

•Non-Contact EF-Detection: An antenna is located along the top-right end of the clamp jaw, which detects electric field surrounds energized conductors. It is ideal for tracing live wiring connections, locating wiring breakage and to distinguish between live or earth connections.

•Probe-Contact EF-Detection: For more precise indication of live wires, such as distinguishing between live and ground connections, use the Red (+) test probe for direct contact measurements.

PC computer interface capabilities

The instrument equips with an optical isolated interface port at the meter back for data communication. Optional purchase PC interface kit BRUA-19X is required to connect the meter to the PC computer RS232 or USB ports. Press and hold the **HOLD** button while turning the meter on to enable meter PC-COMM output.


Hold

The hold feature freezes the display for later view. Press the **HOLD** button momentarily and release to toggle the hold feature.


5ms CREST-MAX capture mode

Press **CREST** (HOLD) button for one second or more and release to activate CREST-MAX capture (Instantaneous Peak-Hold) mode to capture signal peak of voltage or current in duration as short as 5ms. The LCD "**C**" & "**MAX**" turn on. Press again the button momentarily and release can toggle the combination use of HOLD feature. Press the button for 1 second or more and release to exit CREST-MAX capture mode. Auto-ranging and Auto-Power-Off are disabled automatically in this mode.

Electric Field EF-Detection

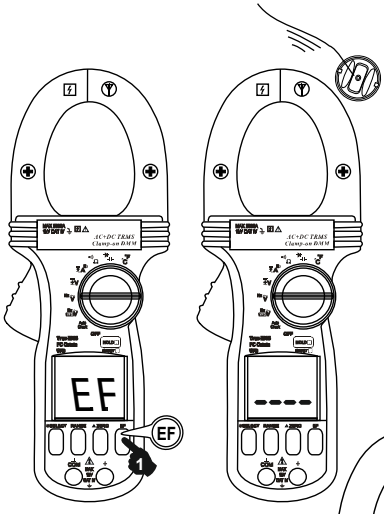

In Voltage or Current function, press the EF button for one second or more and release to toggle to EF-Detection feature. The meter displays "**E.F.**" when it is ready. Signal strength is indicated as a series of bar-graph segments on the display together with variable beep tones.

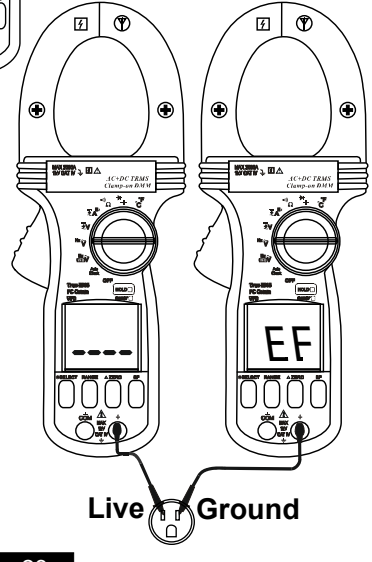

SPECIAL FEATURES:

- AutoCheck ™ Voltage & Ohms
- VFD-V & VFD-Hz function
- 5ms CREST-MAX capture mode (Peak Hold)
- Autoranging Relative -Zero mode & Data Hold function.
- Probe contact, Non-Contact EF-Detection, Diode Test & Continuity Test.
- Backlight LCD Display
- Auto Power Off
- Diode Test & Continuity Test
- PC Interface (Optional)

3) SPECIFICATIONS :

GENERAL SPECIFICATIONS :


- **Sensing :** TRMS sensing
- **Jaw Opening :** 55mm max.
- **Display :** 3-5/6 digits 6000 counts backlight LCD display & 3½ digits 1,999 counts for Hz secondary display.
- **Update Rate :** 5 per second nominal
- **Polarity :** Automatic
- **Low Battery :** Below approx 2.4V
- **Operating Temperature :** 0°C to 40°C
- **Relative Humidity :** Maximum 80% R. H. for temperature upto 31°C decreasing linearly to 50% Relative Humidity at 40°C
- **Storage Temperature :** -20°C to 60°C, < 80% R.H. (With battery removed)
- **Altitude :** Operating below 2000m
- **Temperature Coefficient :** nominal 0.15 x (specified accuracy) / °C @ (0°C--18°C or 28°C--40°C), or otherwise specified

- ✶ **Power supply :** Standard 1.5V AA Battery x 2.
- ✶ **Power Consumption :** Typical 14mA for Current function, & 5.2mA for others.
- ✶ **APO Timing :** Idle for 34 minutes
- ✶ **APO Consumption :** 10μA typical
- ✶ **Dimension :** 264(L) x 97(W) x 43(H) mm
- ✶ **Weight :** Approx. 608gm.
- ✶ **Accessories :** Test leads (pair), user's manual, Bkp60 banana plug K-type Thermocouple x 1 & carrying case.
- ✶ **Optional Accessories :** USB interface kit BRUA-19X, BKB32 banana plug to type-K socket plug adaptor


SAFETY :


- Double insulation per UL/IEC/EN61010-1 Ed. 3.0, IEC/EN61010-2-033 Ed.1.0, CAN/CSA C22.2 No.61010.1 Ed.3.0, IEC/EN61010-2-032 Ed.3.0 & IEC/EN61010-031 Ed.1.1 to CAT IV 1000V AC/DC.
- **Transient Protection :** 12 kV (1.2/50μs surge)
- **Overload Protection :**
  Clamp-on jaws : 2000A DC/AC rms continuous
  Voltage function via terminals : 1100VDC/VAC rms
  " + " & COM Terminals (all other functions) : 1000V DC/AC rms.
- **Pollution degree :** 2
- **EMC :** Meets EN61326-1:2006 (EN55022,EN61000-3-2, EN61000-3-3, EN61000-4-2, EN61000-4-3, EN61000-4-4, EN61000-4-5,EN61000-4-6, EN61000-4-8,EN61000-4-11)
  In an RF field of 3V/m :
  Capacitance function is not specified
  Other function ranges : Total Accuracy = Specified Accuracy + 200 digits
  Performance above 3V/m is not specified.

Temperature Function

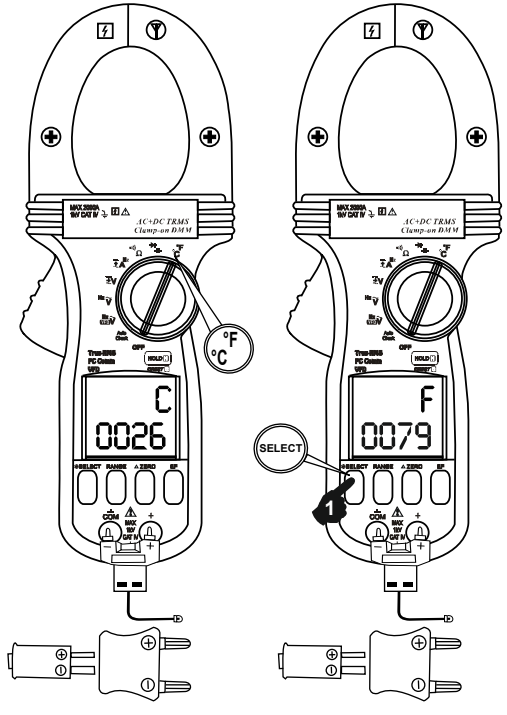

Defaults at °C (Celsius) readings. Press SELECT button momentarily and release to select °F (Fahrenheit) readings. Inputs are made through the test leads terminals. Be sure to insert the banana plug type-K temperature bead probe Bkp60 with correct ± polarities. You can also use a plug adapter bkb32 (optional purchase) with banana pins to type-k socket to adapt other type-k standard mini plug temperature probes.

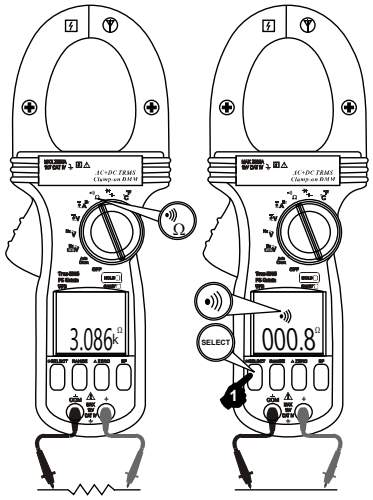

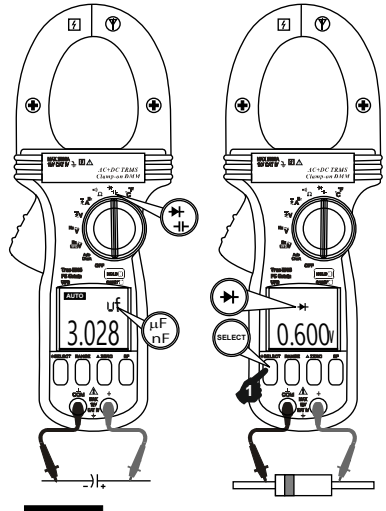

KUSAM-MECO

ELECTRICAL SPECIFICATIONS :

Accuracy is ± (% readings digits + number of digits) or otherwise specified, at 23°C ± 5°C & less than 75% R.H.

True RMS Model KM 2777 accuracies are specified from 5% to 100% of range or otherwise specified. Maximum Crest Factor <1.4:1 at full scale & <2.8:1 at half scale, & with frequency components within the specified frequency bandwidth for non-sinusoidal waveforms.

ACA CURRENT(Clamp on)

Range	Resolution	Accuracy[1)]
50Hz – 60Hz		
200.0 A	100 mA	±(2.0%rdg + 5dgts)
0 ~ 500 A	1 A	±(2.5%rdg + 5dgts)
500~2000 A	1 A	±(3.0%rdg + 5dgts)
40Hz~50Hz & 60Hz~400Hz		
200.0 A	100 mA	±(2.5%rdg + 5dgts)
0 ~ 500 A	1 A	±(3.0%rdg + 5dgts)
500~1000 A	1 A	±(3.5%rdg + 5dgts)
1000~2000 A	1 A	Unspecified

True RMS Crest Factor :
< 1.4:1 at full scale & <2.8:1 at half scale

[1)]Induced error from adjacent current carrying conductor :
<0.1A/A

DCA CURRENT(Clamp on)

Range	Resolution	Accuracy[1)2)]
200.0 A	100 mA	±(2.0%rdg + 5dgts)
0 ~ 500 A	1 A	±(2.0%rdg + 5dgts)
500~2000 A	1 A	±(3.0%rdg + 5dgts)

[1)]Induced error from adjacent current carrying conductor : <0.1A/A

[2)]Specified with Relative Zero Δ mode applied to offset the non-zero residual readings, if any.

DC + ACA CURRENT(Clamp on)

Range	Resolution	Accuracy[1)2)]
DC, 50Hz ~ 60Hz		
200.0 A	100 mA	±(3.0%rdg + 8dgts)
2000 A	1 A	
40Hz ~ 50Hz & 60Hz ~ 400Hz		
200.0 A	100 mA	±(3.5%rdg + 8dgts)
0 ~ 1000 A	1 A	
1000~2000 A	1 A	Unspecified

True RMS Crest Factor :
< 1.4:1 at full scale & <2.8:1 at half scale

[1)]Induced error from adjacent current carrying conductor : <0.1A/A

[2)]Specified with Relative Zero Δ mode applied to offset the non-zero residual readings, if any.

Adjacent current-carrying devices such as transformers, motors and conductor wires will affect measurement accuracy. Keep the jaws away from them as much as possible to minimize influence.

WARNING

Do not use the meter to measure currents above the rated frequency (400Hz). Circulating currents may cause the magnetic circuits of the Jaws reach a hazardous temperature.

Ω Resistance & •)) Continuity Functions

Inputs are made through the test leads terminals. Defaults at Ω **RESISTANCE**. Press **SELECT** button momentarily and release to select. •)) Continuity.

⊣⊢ Capacitance & ⊣▶ Diode functions

Inputs are made through the test lead terminals. Defaults at ⊣⊢ Capacitance. Press **SELECT** button momentarily and release to select ⊣▶ Diode.


Note

When using Diode test function, normal forward voltage drop (forward biased) for a good silicon diode is between 0.400V to 0.900V. A reading higher than that indicates a leaky diode (defective). A zero reading indicates a shorted diode (defective). An OL indicates an open diode (defective). Reverse the test leads connections (reverse biased) across the diode. The digital display shows OL if the diode is good. Any other readings indicate the diode is resistive or shorted (defective).

CAUTION

1. Using Resistance, Continuity, Diode or Capacitance function in a live circuit will produce false results and may damage the meter. In many cases the suspected component (s) must be disconnected from the circuit to obtain an accurate measurement reading.

2. When using Capacitance function, discharge capacitor(s) before making any measurements. Large value capacitors should be discharged through an appropriate resistance load

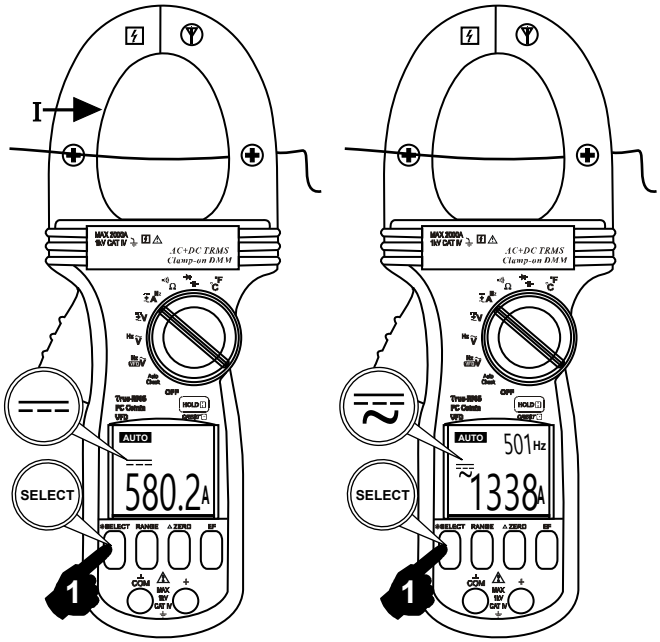

CAUTION (Application and removal of the Clamp-on meter)

For non-invasive current measurements, press the jaw trigger and clamp the jaws around conductor(s) of only one single pole of a circuit for load current measurement. Make sure the jaws are completely closed, or else it will introduce measurement errors. Enclosing conductor(s) of more than one pole of a circuit may result in differential current (like identifying leakage current) measurement. Locate the conductor(s) at the Jaws center as much as possible to get the best measuring accuracy. For removal, press the jaw trigger and remove the jaws from the conductor(s).

DC VOLTAGE

Range	Resolution	Accuracy
6.000 V	1 mV	±(0.5%rdg + 5dgts)
60.00 V	10 mV	
600.0 V	100 mV	
1000 V	1 V	

Input Impedance : 10MΩ, 50pF nominal

AC VOLTAGE

Range	Resolution	Accuracy
50Hz ~ 400Hz		
6.000 V	1 mV	±(1.2%rdg + 5dgts)
60.00 V	10 mV	
600.0 V	100 mV	
1000 V	1 V	

Input Impedance : 10MΩ, 50pF nominal

AC + DC VOLTAGE

Range	Resolution	Accuracy
DC, 50Hz ~400Hz		
6.000 V	1 mV	±(1.4%rdg + 7dgts)
60.00 V	10 mV	
600.0 V	100 mV	
1000 V	1 V	

Input Impedance : 10MΩ, 50pF nominal

VFD_ ACV (with Low Pass Filter)


Range	Resolution	Accuracy [1]
10Hz ~ 20Hz		
6.000 V	1 mV	±(4%rdg + 80dgts)
60.00 V	10 mV	
600.0 V	100 mV	
1000 V	1 V	
20Hz ~ 200Hz		
6.000 V	1 mV	±(2%rdg + 60dgts)
60.00 V	10 mV	
600.0 V	100 mV	
1000 V	1 V	
200Hz~400Hz[2]		
6.000 V	1 mV	±(7%rdg + 80dgts)
60.00 V	10 mV	
600.0 V	100 mV	
1000 V	1 V	

[1] Not specified for fundamental frequency > 400Hz

[3] Accuracy linearly decreases from 2% + 60d @ 200Hz to 7% + 80d @ 400Hz


CREST-MAX CAPTURE MODE

Accuracy :
Specified accuracy plus 250 digits for changes > 5ms in duration

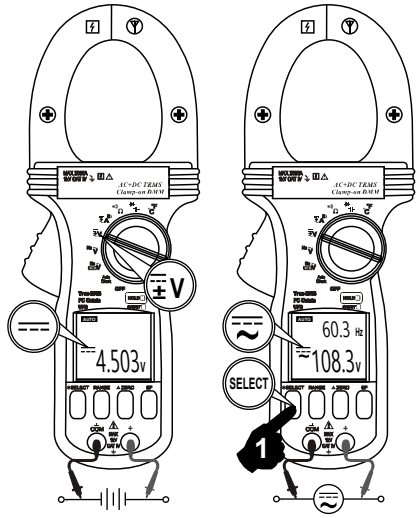

ACA Hz, DCA & DC+ACA Hz functions

Input is made through the clamp jaws for non-invasive current measurements. Defaults at **ACA Hz** function. Press **SELECT** button momentarily & release to select the subject functions in sequence.

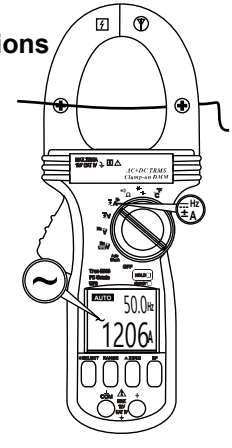

VFD-ACV^{Hz} & ACV^{Hz} functions

Inputs are made through the test leads terminals.


VFD-ACV^{Hz} function is to deal with VFD (Variable Frequency Device) signals. It, however, further pre-selects the most appropriate voltage-ranges and thus the Hz trigger levels to best cope with most VFD-Voltage and VFD-Frequency applications.

Note: The Hz trigger level is determined by the **AC/DC+AC Voltage or Current** function-range being in use. Press **RANGE** button to select different function-ranges and thus trigger levels manually.

DCV & DC+ACV^{Hz} functions

Inputs are made through the test leads terminals. Defaults at **DCV** Function.

Press **SELECT** button momentarily and release to select **DC+ACV^{Hz}**.

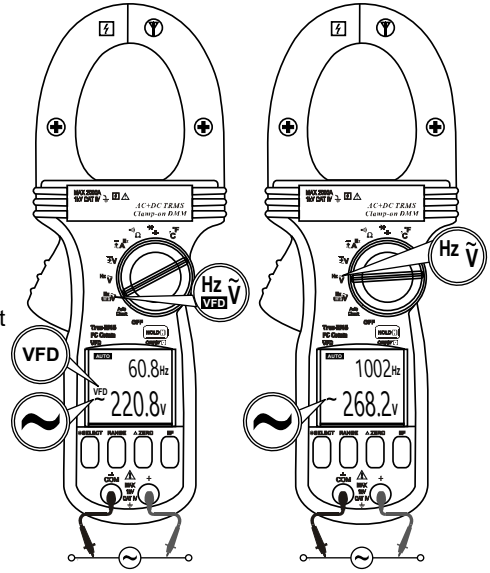

NON-CONTACT EF-DETECTION

Typical Voltage	Bar-Graph Indication
89V (tolerance : 12V ~ 165V)	-
177V (tolerance : 81V ~ 272V)	- - -
589V (tolerance : 178V ~ 1000V)	- - - - -

Indication : Bar-graph segments & audible beep tones proportional to the field strength

Detection Frequency : 50/60Hz

Detection Antenna : Top side of the stationary jaw

Probe-Contact EF-Detection: For more precise indication of live wires, such as distinguishing between live and ground connections, use the Red (+) test probe for direct contact measurement.

CAPACITANCE

Range	Resolution	Accuracy [1]
60.00 nF	10 pF	±(2.0%rdg + 5dgts)
600.0 nF	100 pF	
6.000 μF	1 nF	
60.00 μF	10 nF	±(3.5%rdg + 5dgts)[2]
600.0 μF	100 nF	
2000 μF	1 μF	±(4.0%rdg + 5dgts)[2]

[1] Accuracies with film capacitor or better

[2] Temperature Coefficient : 0.25 x (specified accuracy) / °C @ (0°C ~ 18°C or 28°C ~ 40°C)

AUTOCHECK™_DCV

Range	Resolution	Accuracy
6.000 V	1 mV	±(1.3%rdg + 5dgts)
60.00 V	10 mV	
600.0 V	100 mV	
1000 V	1 V	

AutoCheck™ Lo-Z DCV Threshold : >+1.5VDC & <-1.5VDC nominal.

AutoCheck™ Lo-Z DCV input impedance :

Initially approx. 2.5kΩ, 600pF nominal; impedance increases abruptly within a fraction of a second as display voltage is above 50V (typical).

Ended up impedances vs display voltages typically are :

10 kΩ @ 100V

60 kΩ @ 300V

200kΩ @ 600V

420kΩ @ 1000V

OHM & AUTOCHECK™ _OHM[1)]

Range	Resolution	Accuracy
600.0 Ω	0.1 Ω	±(0.5%rdg + 5dgts)
6.000 KΩ	1 Ω	
60.00 KΩ	10 Ω	
600.0 KΩ	100 Ω	±(0.8%rdg + 5dgts)
6.000 MΩ	1 KΩ	±(1.2%rdg + 5dgts)
40.00 MΩ	10 KΩ	±(2.3%rdg + 5dgts)

Open Circuit Voltage : 0.45VDC typical.

[1)]**AutoCheck™ OhmThreshold :** <10.00MΩ nominal.

Note:

***Range-Lock and Function-Lock Feature:** When a measurement reading is being displayed in **AutoCheck™** mode, press the **RANGE** or **SELECT** button momentarily 1 time can lock the range or function it was in. Press the button momentarily repeatedly to step through the ranges or functions.

***As Hazardous-Alert** : When making resistance measurements in **AutoCheck™** mode, an unexpected display of voltage readings alerts you that the object under test is being energized.

***Ghost - voltage Buster** : Ghost - voltages are unwanted stray signals coupled from adjacent hard signals, which confuse common multimeter voltage measurements. Our AutoCheck™ mode provides low (ramp-up) input impedance (approx. 2.5kΩ at low voltage) to drain ghost voltages leaving mainly hard signal values on meter readings. It is an invaluable feature for precise indication of hard signals, such as distinguishing between hot and open wires (to ground) in electrical installation applications.

WARNING:


AutoCheck™ mode input impedance increases abruptly from initial 2.5kΩ to a few hundred kΩ's on high voltage hard signals. "**LoZ**" displays on the LCD to remind the users of being in such low impedance mode. Peak initial load current, while probing 1000VAC for example, can be up to 566mA (1000V x 1.414 / 2.5kΩ), decreasing abruptly to approx. 3.37mA (1000V x 1.414 / 420kΩ) within a fraction of a second. Do not use AutoCheck™ mode on circuits that could be damaged by such low input impedance. Instead, use rotary-switch selector $\tilde{\mathbf{V}}$ or $\overline{\tilde{\mathbf{V}}}$ high input impedance voltage modes to minimize loading for such circuits.

OPERATION

CAUTION : *Before and after hazardous voltage measurements, test the voltage function on a known source such as line voltage to determine proper meter functioning.*

AutoCheck™ mode

This innovative **AutoCheck™** feature automatically selects measurement function of **ACV** ^{Hz}, **DCV**, or **Resistance (Ω)** based on the input via test leads.

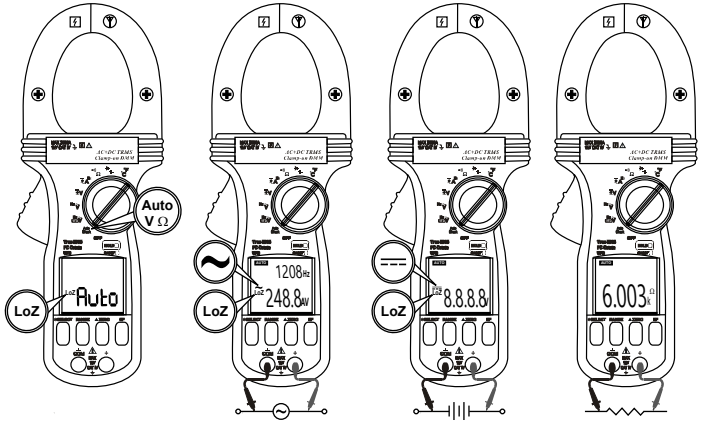

- With no input, the meter displays “Auto” when it is ready.
- With no voltage signal but a resistance below 10M (nominal) is present, the meter displays the resistance value. When the resistance is below the “Audible Threshold”, the meter further gives a continuity beep tone.
- When a signal above the voltage threshold of 1.5V DC or AC up to the rated 1000V is present, the meter displays the voltage value in appropriate DCV or ACV, whichever larger in peak magnitude.

~Hz LINE LEVEL FREQUENCY

Function		Sensitivity (Sine RMS)	Range
6	V	2 V[2)]	40Hz ~ 1999Hz
60	V	20 V[2)]	40Hz ~ 1999Hz
600	V	100 V[2)]	40Hz ~ 1999Hz
1000	V	600 V[3)]	40Hz ~ 1999Hz
200	A	10 A[2)]	20Hz ~ 400Hz
2000	A	100 A[2)]	20Hz ~ 400Hz
VFD 6	V[1)]	0.6V ~ 2.4V[2)]	10Hz ~ 400Hz
VFD 60	V[1)]	6~24V[2)]	10Hz ~ 400Hz
VFD 600	V[1)]	60V ~ 240V[2)]	10Hz ~ 400Hz

Accuracy : 0.1% + 4d

[1)]VFD sensitivity linearly decreases from 10% F.S. @ 200Hz to 40% F.S. @ 400Hz

[2)]DC-bias, if any, not more than 50% of Sine RMS

[3)]DC-bias, if any not more than 100V

DIODE TESTER

Range	Test Current (Typical)	Open Circuit Voltage
1.000V	0.56mA	<1.8V DC typical

Accuracy : 1.0% + 3d

AUTOCHECK™_ACV

Range	Resolution	Accuracy [1]
50Hz ~ 60Hz		
6.000 V	1 mV	±(1.5%rdg + 5dgts)
60.00 V	10 mV	
600.0 V	100 mV	
1000 V	1 V	

AutoCheck™ Lo-Z ACV Threshold : >1.5V (50/60Hz) nominal.

AutoCheck™ Lo-Z ACV input impedance :

Initially approx. 2.5kΩ, 600pF nominal; impedance increases abruptly within a fraction of a second as display voltage is above 50V (typical). Ended up impedances vs display voltages typically are :

10 kΩ @ 100V
60 kΩ @ 300V
200kΩ @ 600V
420kΩ @ 1000V

TEMPERATURE


Range	Resolution	Accuracy
-50°C ~ 1000°C	1°C	±(0.3%rdg + 4dgts)
-58°F ~ 1832°F	1°F	±(0.3%rdg + 6dgts)

K-type Thermocouple range & accuracy not included

AUDIBLE CONTINUITY TESTER

Audible Threshold	Response Time
between 10Ω and 200Ω	32ms approx.

PRODUCT DESCRIPTION

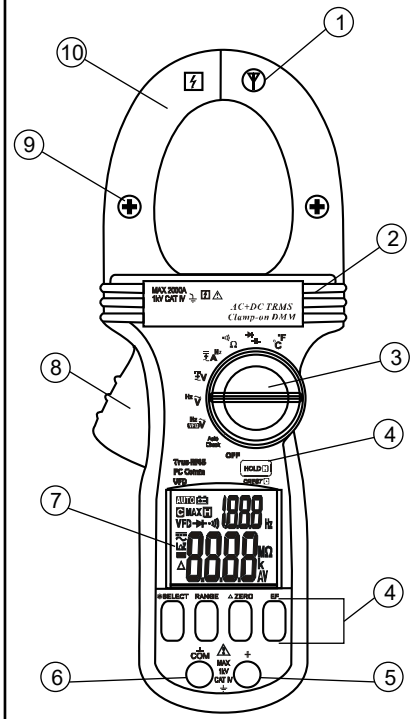

1) Antenna for Non-Contact EF-Detection
2) Hand/Finger Barrier to indicate the limits of safe access of the meter during measurement
3) Rotary-switch Selector to turn the power ON/OFF and Select a function
4) Push-buttons for special functions & features.
5) Input Jack for all functions EXCEPT non-invasive DCA & ACA current functions
6) Common (Ground reference) Input Jack for all functions EXCEPT non-invasive DCA & ACA current functions
7) 3-5/6 digits 6000 counts & 3-1/2 digits 2000 counts dual numeric LCD display
8) Jaw trigger for opening the clamp jaw
9) Jaw center (& DCA polarity) Indicator, at where best DCA & ACA accuracy is specified
10) Hall-effect Clamp Jaw for AC & DC current magnetic field pick up.