KUSAM-MECO®

An ISO 9001:2015 Company

KM 2779

Operating Manual



2500A Digital Clamp Meters

DATE:2021.08.21
REV.1

KUSAM-MECO®
An ISO 9001:2015 Company

CONTENTS

I. OVERVIEW---------- 1
II. OPEN CASE AND CHECK---------- 1
III. SAFETY CODES----------2
IV. ELECTRICAL SYMBOLS ---------- 3
V. EXTERNAL STRUCTURE ---------- 4
VI.LCD DISPLAY ---------- 5
VII.KEY FUNCTION ---------- 7
VIII.MEASUREMENT OPERATING INSTRUCTION ---------- 9
1. DC voltage measurement ---------- 9
2. AC voltage measurement ----------11
3. Resistance measurement ----------13
4. Circuit on-off measurement----------15
5. Diode measurement ----------17
6. Capacitance measurement ----------19
7. Frequency/duty ratio measurement ----------21
8. Temperature measurement----------23
9. DC current measurement ---------- 25
10.AC current measurement ----------27
11. Current signal output function ---------- 29
12.Power gear ----------30
13. Automatic shutdown function----------30
IX. TECHNICAL INDICATOR ----------31
X. MAINTENANCE AND UPKEEP ----------39

I. OVERVIEW

KM 2779 is a portable true RMS 3-5/6 bit (6000 Counts), auto range clamp ammeter with simulation bar. The clamp ammeter featuring full-function on screen display, full-range overload protection and unique appearance design has become a specific clamp ammeter with superior performance. The clamp ammeter is applicable to following measurements: AC/DC voltage, AC/DC current, surge current, resistance, frequency, maximum/minimum value measurement, relative value measurement, data recording and read-back, under-voltage di splay and automatic shutdown function.

The instruction manual includes relevant safety information and warning indication, please read them carefully and strictly observes all warnings and notes.

II. OPEN CASE AND CHECK

Unpack and take out the instrument, please check carefully if the following attachment are complete or intact, if any lack or damage were found, please contact with your supplier.

- ●An operating instruction manual
- ●A test pen
- ●A temperature sensor
- ●A tool box
- ●A certificate

Optional Components:

- ●Analog output line

KUSAM-MECO®
An ISO 9001:2015 Company

III. SAFETY CODES

The clamp ammeter is designed and produced strictly in accordance with IEC61010-1 safety standard. It meets the double insulation over-voltage standard CAT Ⅲ 1000V, CAT Ⅳ 600V and safety standards of pollution degree Ⅱ. If fail to use the meter under the relevant operation Instruction, the protection provided shall be weakened or lost.

1. Check the clamp ammeter and test pen before using, guard against any damage or abnormal phenomenon. If any abnormal condition were found: bare test pen, damaged chassis, no display or random display in LCD, please do not use it. It is forbidden to use the clamp ammeter without rear cap or rear cap not in place, or otherwise there will be electric shocking.
2. Damaged test pen should be replaced with the one of same type or electric specification.
3. Do not contact the bare wire and connector, unused input terminal or the circuit being measured when clamp ammeter is in operation.
4. Be careful in measuring voltage higher than DC 42V or AC 30V and keep finger within the scope of test pen finger protection position to guard against electric shocking.
5. Set the function range switch at the maximum range position if the scope of measured value couldn't be defined.
6. Refrain from applying between terminals or the terminals and grounding the voltage or current over the rating value labeled on the clamp ammeter.
7. Function switches shall be set at the correct position in measurement. Before converting function switches, connection between the table pen measured circuits shall be broken off and gear conversion in measurement shall be prohibited to guard against damage to the meter.

8. Refrain from storing or using the clamp ammeter in the explosive and flammable environment with high temperature, high humidity and strong electromagnetic field.
9. Refrain from changing the internal wiring in the clamp ammeter to guard against damage to the meter and danger.
10. When LCD display shows the icon “ ” , it is required to replace the battery in time to ensure the measurement accuracy.
11. Power off immediately after measurement. Take out battery when the clamp ammeter will not be in use for a long time.
12. Probe assemblies to be used for MAINS measurements shall be RATED as appropriate or MEASUREMENT CATEGORY III 1000V or IV 600V according to IEC 61010-031 and shall have a voltage RATING of at leat the voltage of the circuit to measured.
13. CAT III: MEASUREMENT CATEGORY III (CAT III) is applicable to test and measuring circuits connected to the distribution part of the building’s low-voltage MAINS installation.
14. CAT IV: MEASUREMENT CATEGORY IV (CAT IV) is applicable to test and measuring circuits connected at the source of the building’s low-voltage MAINS installation.
15. Please check whether the instrument is in good condition before use,such as test the voltage which is known and confirm the readings are accurate.

Conforms to UL STD. 61010-1, 61010-2-030, 61010-2-032, 61010-2-033, Certified to CSA STD. C22.2 NO. 61010-1, 61010-2-030, IEC STD 61010-2-032, IEC STD 61010-2-033


KUSAM-MECO®
An ISO 9001:2015 Company

IV. Electrical symbols


	Diode		Earth(ground) TERMINAL
	Low battery		Equipment protected throughout by DOUBLE INSULATION or REINFORCED INSULATION
	Caution		Both direct and alternating current
	Alternating current		Caution, possibility of electric shock
	Direct current	CE	Comply with EU standard
	Buzzing on-off		

V. EXTERNAL STRUCTURE (SEE FIGURE 1)

1. Hand Guards:to protect user s hand from touching the dangerous area.
2. Clamp head pulling handle：Press the trigger to open the clamp head, when release the trigger, clamp head will partially closed.
3. Functional key： Select basic functions.
4. Analog current output
5. Measure input termina： Measure the signal inputl.
6. Toggle：Used to select the measurement of input terminal or analog current output terminal.

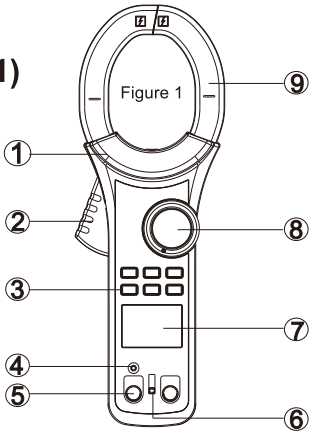

7. LCD display area：Display the measurement data and functional symbols.
8. Dial switch： Select the measurement function gear.
9. Clamp head：A device used to measure AC/DC current and covert current into voltage.

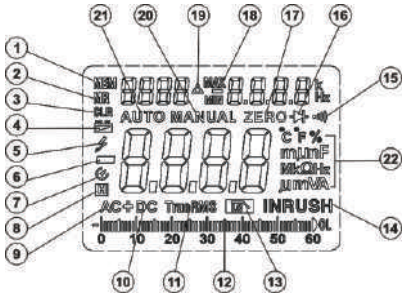


VI. LCD DISPLAY (SEE FIGURE 2)

1.MEM:	Memory number prompt
2.MR	Read back stored data prompt
3.CLR	Stored data clearing prompt
4.	Battery under-voltage prompt
5.	High voltage warning prompt
6.	Display negative reading
7.	Auto shutdown prompt
8.	Hold mode prompt

KUSAM-MECO®
An ISO 9001:2015 Company

9.AC	AC measurement prompt	
10.DC	DC measurement prompt	
11.TrueRMS	TrueRMS measurement prompt	
12.＋system digit and simulation bar	Measurement of reading value	
13.	LPF measurement prompt	
14.INRUSH	INRUSH current measurement prompt	
15.	Buzzing on-off measurement prompt	
16.	Diode measurement prompt	
17.ZERO	AC current gear ZERO prompt	
18.MAX、MIN	Maximum and minimum value measurement prompt	
19.△	Relative measurement prompt	
20.Manual	Manual range prompt	
21.Auto	Auto range prompt	
22.Measurement unit:	V	Voltage unit: Volt
	A	Current unit: Ampere
	Ω、kΩ、MΩ	Resistance unit:Ω,kΩ,MΩ
	nF、μF、mF	Capacitance unit:nF,μF,mF
	Hz、kHz、MHz	Frequency unit:Hz,kHz,Mhz
	℃、℉	Temperature unit:℃,℉

VII. KEY FUNCTION (SEE FIGURE 3)

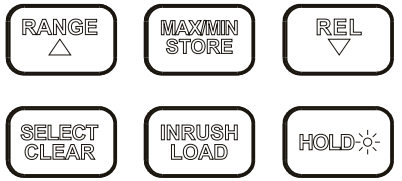

1.SELECT/CLEAR

It is able to select gear by a short press.

With a long press, LCD will display “CLR” symbol, clear stored data record, and then “CLR” symbol disappears, MEM stored number becomes 0.

2.RANGE/▲

Under the non-read back storage of record data mode, enter the manual measurement mode by a short press on RANGE and change the range. After a long press on RANGE, manual range will turn to auto range.

Under the read back storage record data mode, it is able to read back the upward data by pressing the key.

3.MAX/MIN/STORE

With a press on the key, enter MAX/MIN standby mode, LCD will display “————”; after the second press, LCD will display “MAX” to enter the maximum value measurement mode, after

KUSAM-MECO®
An ISO 9001:2015 Company

the third press, LCD will display “MIN” to enter the minimum value measurement mode. Under non-standby mode, it is able to record the current measurement data with a long press on the key.

4.REL/▲

With the exception of DC current gear, under the non-read back stored record data mode, it is able to enter the relative measurement mode with a short press, the main display will show: measured value-basic value, the right display: basic value, after another press, quit the mode.

Under the DC gear measurement mode, enter the clearing mode with a short press, LCD will display “ZERO”.

Under the non-read back stored record data mode, it is able to enter the continuous recording data mode, after another long press, quit the mode.

Under the read back stored recording data mode, it is able to read back the recorded data backward by pressing the key.

5. INRSUH/LOAD

At the AC current gear, it is able to enter INRUSH current measurement mode by pressing the key, after another pressing, quit the mode.

After long press on the key, enter the read back stored recording data mode, after another press on the key, quit the mode.

6. HOLD/☼

After a short press, enter the reading hold measurement mode, after another press, quit the mode.

After a long press, the backlight will be illuminated, in case of long press within 10s, backlight will be out, and if no long press, it will be automatically out after 10s.

VIII. MEASUREMENT OPERATING INSTRUCTION

1. DC voltage measurement (See Figure 4)

1) Insert red test pen in “V” jack and black test pen in “COM” jack.
2) Push the function range switch to the DC voltage measurement gear, and connect test pen in parallel with the power or load to be measured.
3) Directly read the measured voltage value from display.
4) Press SELECT at the DC voltage measurement gear to select AC+DC measurement.

⚠ Note:

- Do not input voltage higher than 1000V. It may be feasible to measure higher voltage, but damage will be caused to the meter.
- Watch out for electricity shocking when measuring high voltage.
- After completing all measurement operations, disconnect test pen from the measured circuit.
- When measured voltage is higher than the safety voltage 42V/DC, the meter LC displays high voltage warning prompt “ ⚡”; when inputting overvoltage, higher than DC 1000V gear range, the meter ⚡ will automatically sound intermittent buzzing and high voltage warning prompt will automatically flash to provide warning prompt.

KUSAM-MECO®
An ISO 9001:2015 Company

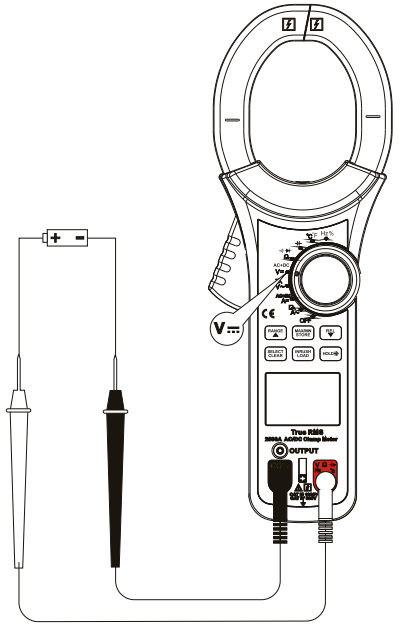


Figure 4

2. AC voltage measurement (See Figure 5)

1) Insert red test pen in “V” jack and black test pen in “COM” jack.
2) Push the function range switch to the DC voltage measurement gear, and connect test pen in parallel with the power or load to be measured.
3) Main display will show the true RMS, while the right secondary display shows frequency value. Conditions must be met when reading frequency value: input range ≥ range × 10%.
4) Press SELECT at the AC voltage measurement gear to select LPF measurement LO.

⚠ Note:

- Pay attention to the electric shock in measuring high voltage.
- After completing all measurement operations, disconnect test pen from the measured circuit.
- When measured voltage is higher than the safety voltage 30V/AC, the meter LC displays high voltage warning prompt “⚡”; when inputting overvoltage, higher than AC 1000V gear range, The meter will automatically sound intermittent buzzing and high voltage warning prompt will ⚡ automatically flash to provide warning prompt.
- AC conversion adopts the AC coupling true RMS response mode, sinusoidal input for correction. The accuracy of non-sinusoidal wave shall be adjusted as follows:

Crest factor 1.4～2.0, accuracy should be increased 1.0%;
Crest factor 2.0～2.5, accuracy should be increased 2.5%;
Crest factor 2.5～3.0, accuracy should be increased 4.0%;

KUSAM-MECO®
An ISO 9001:2015 Company

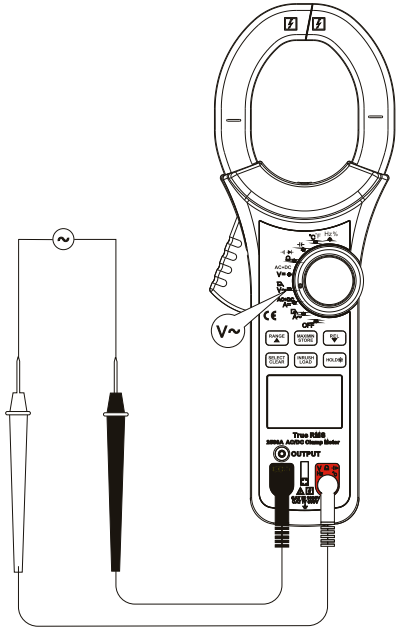


Figure 5

3. Resistance measurement (See Figure 6)

1) Insert red test pen in “Ω” jack and black test pen in “COM” jack.
2) Push the function range switch to the measurement gear “Ω” press SELECT to select resistance measurement Ω and connect test pen in parallel with the two terminals of measured resistance .
3) Directly read the measured resistance value from display.

⚠ Note:

- If the resistance open circuit or resistance being measured exceeds the maximum range of the meter, display will show “OL”.
- Before measuring resistance on-line, the power of circuits being measured shall be powered off and all capacitors shall release out residues of electric charges to assure the measurement accuracy.
- When measuring low resistance, a measurement error of 0.1Ω～0.2Ω will be caused to the test pen, to acquire the accurate reading, it is able to utilize the relative measurement function, input test pen under short-circuit condition, press the ▲ , carry out low resistance measurement after the meter automatically deducts the test pen displayed value under short-circuit condition.
- If the resistance value is not less than 0.5Ω when table pen is short circuited, please inspect test pen for loosening or other reasons.
- In measuring resistance over 1MΩ, it might take several seconds to stabilize the reading, it is normal for high resistance measurement. To acquire stable reading, the test short line can be used for measurement.
- Do not input voltage higher than DC 42V or AC 30V, which may cause personal injury.
- After completing all measurement operations, disconnect the test pen from the circuit being Measured.

KUSAM-MECO®
An ISO 9001:2015 Company

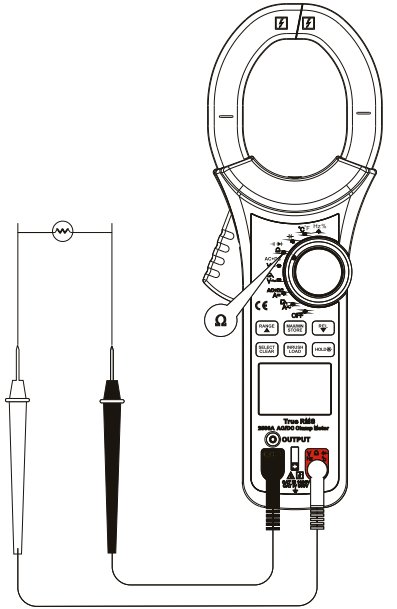


Figure 6

4. Circuit on-off measurement •)) (See Figure 7)

1) Insert red test pen in “Ω” jack and black test pen in “COM” jack.
2) Push the function range switch to the measurement gear “Ω•))►|” , press SELECT to select circuit on-off measurement and connect test pen in parallel with the two terminals of measured circuit. When the measured resistance between two terminals <30Ω, the circuit should be deemed conductive, buzzer will sound continuously. When resistance is ≥30Ω, the buzzer will not sound.
3) Directly read the measured resistance value loaded by the circuit from display.

⚠ Note:

- When checking on-line circuit on-off condition, it is required, prior to measurement, to power off all powers in the measured circuit, and discharges all residual charges in the capacitor.
- With respect to the circuit on-off measurement, open-circuit voltage is approximately -3.5V and range should be 600Ω measurement gear
- Do not input voltage higher than DC 42V or AC 30V, which may cause personal injury.
- After completing all measurement operations, disconnect the test pen from the measured circuit.

KUSAM-MECO®
An ISO 9001:2015 Company

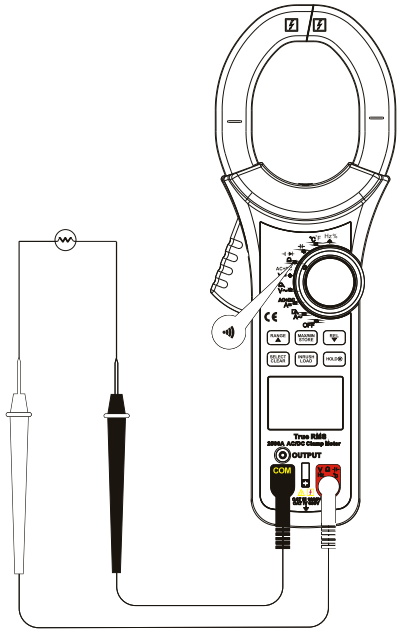


Figure 7

5. Diode measurement ⊣◁ (See Figure 8)

1) Insert red test pen in "⊣◁" jack and black test pen in "COM" jack. Polarity of red and black test pen is respectively "+" and "-".
2) Push the function range switch to the measurement gear "Ω ·)) ⊣◁", press SELECT to select diode measurement and ⊣◁ directly read out the approximate forward direction PN junction voltage.
   For silicon PN junction, generally 500～800mV is confirmed to be the normal value.

⚠ Note:

- "OL" will be displayed when the measured diode is open-circuit or polarity is inversely connected.
- Before measuring diode, the power of circuits being measured shall be powered off and all capacitors shall release out residues of electric charges to assure the measurement accuracy.
- The test open-circuit voltage of diode is approximately 3.5V.
- Do not input voltage higher than DC 42V or AC 30V, which may cause personal injury.
- After completing all measurement operations, disconnect the test pen from the measured circuit.

KUSAM-MECO®
An ISO 9001:2015 Company

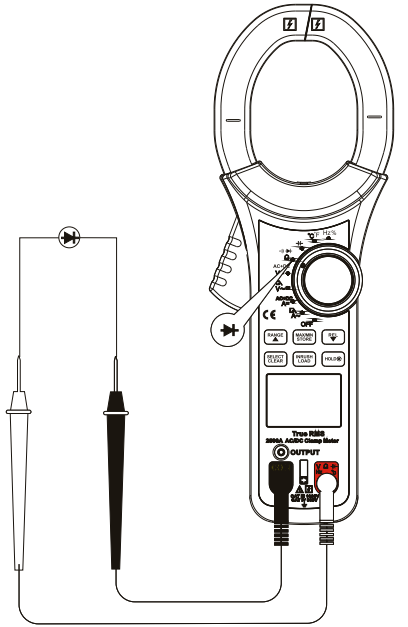


Figure 8

6. Capacitance measurement (See Figure 9)

1) Insert red test pen in "⊣⊢" jack and black test pen in "COM" jack.
2) Push the range switch to the measurement gear "⊣⊢", connect test pen in parallel with the two terminals of measured capacitance.
3) Directly read out the capacitance value of measured circuit from display. It is recommended to carry out capacitance measurement with test short line input, thus reducing the impact caused by distributed capacitance.

⚠ Note:

- If the measured capacitance is short circuited or capacitance exceeds the maximum range of the meter, display will show "OL".
- Under capacitance measurement mode, simulation bar indicator is forbidden. It will take longer time to achieve the correct reading when measuring capacitance larger than 600 μF.
- To ensure the measurement accuracy, it is recommended to discharge all residual charges in the capacitor before test, then input meter for measurement, which is of particular importance to the capacitor with high voltage. It is required to prevent damage to the meter and personal injury.
- After completing measurement operation, disconnect the test pen from the measured capacitance.

KUSAM-MECO®
An ISO 9001:2015 Company

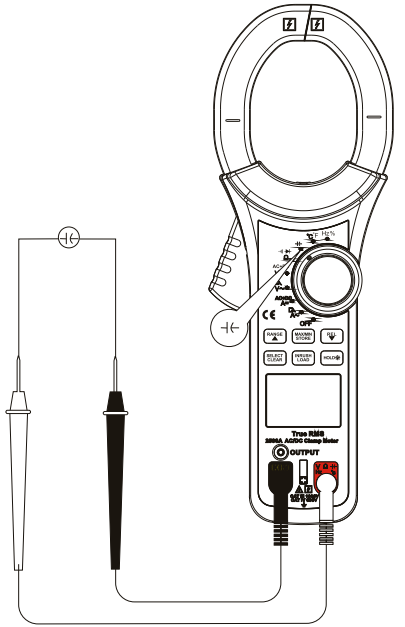


Figure 9

7. Frequency/duty ratio measurement (See Figure 10)

1) Insert red test pen in “Hz” jack and black test pen in “COM” jack.
2) Push the range switch to the measurement gear “mV⎓/Hz%” and press the red key to select Hz function, connect test pen in parallel with the signal source to be measured.
3) Directly read out the measured frequency value from display.
4) Press SELECT to select duty ratio measurement.

⚠ Note:

- a when measuring:
  10Hz～40MHz：1Vrms≤ a ≤30Vrms>40MHz: For reference
- Do not input frequency higher than 30V rms, which may cause personal injury.
- After completing all measurement operations, disconnect the test pen from the measured circuit.

KUSAM-MECO®
An ISO 9001:2015 Company

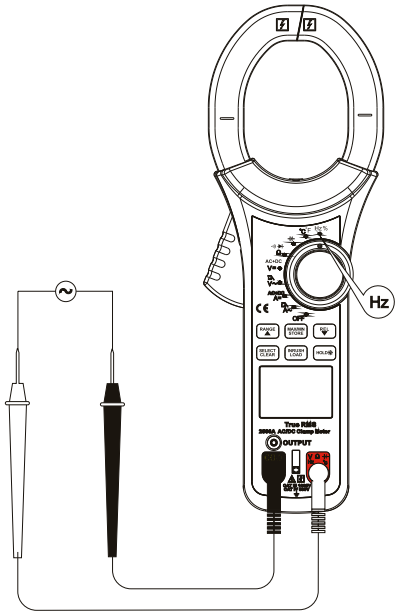


Figure 10

8.Temperature measurement (See Figure 11)

1) Push range switch to “℃ ℉” gear, LCD will display OL, the short-circuit test pen displays the room temperature.
2) Insert temperature K type socket in the corresponding hole as per the diagram.
3) Put temperature robe detect the measured surface, several seconds later, directly read out the measured Celsius temperature value from LCD.
4) Press SELECT to select Fahrenheit temperature measurement.

⚠ Note:

- The meter should not be operated in a place with ambient temperature beyond the range 18-28℃, or otherwise measurement error will be resulted, particularly evident in low temperature environment.
- Do not input voltage higher than DC 42V or AC 30V, which may cause personal injury.
- After completing all measurement operations, take off the temperature probe.

KUSAM-MECO®
An ISO 9001:2015 Company

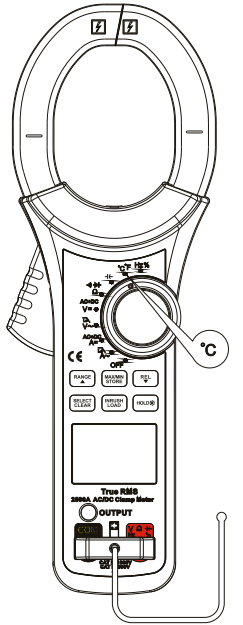


Figure 11

9. DC current measurement (See Figure 12)

1) Push the switch to DC current gear A⎓, when LCD display is not zero, press REL to clear. After measuring big current gear, clamp head will be left with remanence, and LCD display will have base values.
2) Press trigger to open the clamp head to take the conductor to be measured, then slowly loosen the trigger until clamp head is completely closed. Be sure the conductor to be measured is clamped at the center of clamp head, if not, additional error may be resulted, and clamp ammeter can only measure one current conductor, measuring two or more current conductors concurrently may result in wrong measurement reading.
3) Directly read out the measured DC current value from display.
4) Press SELECT at the DC current gear to select AC+DC measurement.

⚠ Note:

- Current measurement must be operated within 0℃～40℃, if positive reading is achieve after measuring DC current, the current direction will be from up to down (See Figure 10: the upward is panel and base cap is downward). Do not loosen trigger abruptly, since Hall component is sensitive in some extent to magnet, heat and mechanical stress, but also to the impact, which may cause short-time reading variation.
- Be sure the conductor to be measured is clamped at the center of clamp head, if not, an additional reading error of ±1.0% may be resulted.

KUSAM-MECO®
An ISO 9001:2015 Company

- Do not use more than 60 Hz maximum rated frequency.

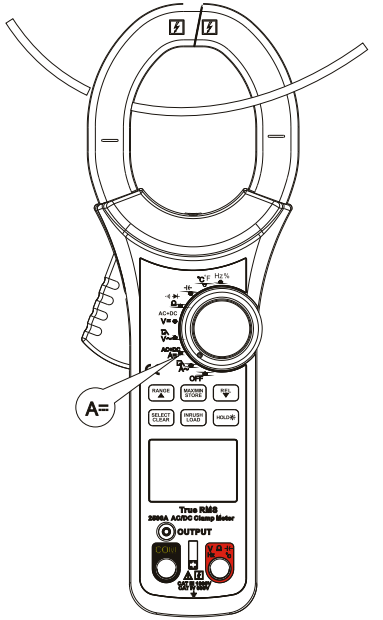


Figure 12

10. AC current measurement (See Figure 13)

1) Push the switch to AC current gear A～, press trigger to open the clamp head to take the conductor to be measured, then slowly loosen the trigger until clamp head is completely closed. Be sure the conductor to be measured is clamped at the center of clamp head, if not, additional error may be resulted, and clamp ammeter can only measure one current conductor, measuring two or more current conductors concurrently may result in wrong measurement reading.
2) Main display will show the true RMS, while the right secondary display shows frequency value. Conditions must be met when reading frequency value: input range ≥range×10%.
3) Press SELECT at the AC voltage measurement gear to select LPF measurement LPF
4) It is able to press INRUSH at AC current gear to select surge current measurement, clamp ammeter displays "----", indicating it is under standby status for measuring surge current. After starting electrical appliance, the instant-on current of appliance can be measured out; press INRUSH key again to quit the surge current measurement. 600A range can be available for surge current measurement.

⚠ Note:

- Current measurement must be operated within 0℃～40℃, if positive reading is achieve after measuring DC current, the current direction will be from up to down (See Figure 10: the upward is panel and base cap is downward). Do not loosen trigger abruptly, since Hall component is sensitive in some extent to magnet, heat and mechanical stress, but also to the impact, which may cause short-time reading variation.
- Be sure the conductor to be measured is clamped at the center of clamp head, if not, an additional reading error of ±1.0% may be resulted
- AC conversion adopts the AC coupling true RMS response mode, sinusoidal input for correction. The accuracy of non-sinusoidal wave shall be adjusted as follows:

KUSAM-MECO®
An ISO 9001:2015 Company

Crest factor 1.4～2.0, accuracy should be increased 1.0%;
Crest factor 2.0～2.5, accuracy should be increased 2.5%;
Crest factor 2.5～3.0, accuracy should be increased 4.0%;

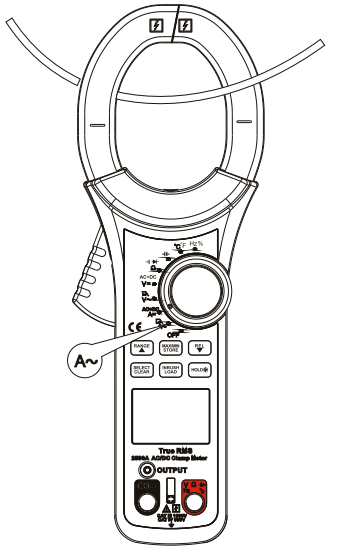


Figure 13

IX. TECHNICAL INDICATOR

1. General specification

- Liquid crystal display: 3 5/6 bit liquid crystal display, maximum display 6000.
- Polarity display: auto positive and negative polarity display.
- Overload display: “OL” or “-OL”.
- Low voltage display: “ ” indicates that batter voltage is lower than working voltage, reminding replacing battery.
- Sampling rate: 3/s
- Type of sensor: Hall effect sensor for DC/AC measurement
- Test position error: an additional reading error of ±1.0% may be resulted when the power to be measured is not clamped at the center of clamp head
- Resistance to impact strength: 1m fall impact
- Maximum openness of clamp head: diameter 63mm
- Maximum size of current lead: diameter 60mm
- Electromagnetic field impact: the application of device near electromagnetic field may result in unstable display or inaccurate reading.
- Power requirement: 6LF22 9V alkaline battery
- Dimension: 298mm×107mm×47mm
- Weight:bout 726g (inclusive of battery);

KUSAM-MECO®
An ISO 9001:2015 Company

2. Environment

Indoor

- Maximum height: 2000m
- Safety code: CAT IV 600, CAT III 1000 pollution grade: 2
- Operating humidity and temperature:
  0℃～30℃(not bigger than 80%RH), 30℃～40℃ (not bigger than 75%RH),
  40℃～50℃(not bigger than 45%RH)
- Storage humidity and temperature: -20℃～+60℃ (not bigger than 80%RH)

3. Electrical specification

- Accuracy: ± (%+ word number), one-year calibration time
- Ambient temperature: 23℃±5℃
- Ambient humidity: ≤80% RH
- Temperature coefficient: 0.1×(accuracy) /℃

(1) DC voltage V⎓

Range	Resolution	Accuracy: ± (% reading + word number)
6V	0.001V	±(0.5%+2)
60V	0.01V	
600V	0.1V	
1000V	1V	±(1%+2)

Input impedance: about 10MΩ
Overload protection: 1000V

(2) AC voltage V~

Range	Resolution	Accuracy: ± (% reading + word number)	
6V	0.001V	40Hz∽400Hz	400Hz∽1kHz
60V	0.01V	±(1%+3)	±(2%+3)
600V	0.1V		
1000V	1V	±(1.2%+3)	±(2.5%+3)

Input impedance: about 10MΩ
Overload protection: 1000V
Display: true RMS, applicable to 10%- 100% of the range.

(3) Voltage AC+DC

Range	Resolution	Accuracy: ± (% reading + word number)	
6V	0.001V	40Hz∽400Hz	400Hz∽1kHz
60V	0.01V	±(2%+20)	±(4%+20)
600V	0.1V		
1000V	1V	±(2.5%+20)	±(5%+20)

Input impedance: about 10MΩ
Overload protection: 1000V
Display: true RMS, applicable to 10%- 100% of the range.

KUSAM-MECO®
An ISO 9001:2015 Company

(4) DC current A⎓

Range	Resolution	Accuracy: ± (% reading + word number)
600A	0.1A	±(1.5%+5)
2500A	1A	±(2.5%+5)

(5) AC current

Range	Resolution	Accuracy: ± (% reading + word number)
600A	0.1A	±(1.5%+5)
2500A	1A	±(2.5%+5)

Display: true RMS, applicable to 10%- 100% of the range.
Frequency response: 50Hz～60Hz
It is normal that the clamp vibrates slightly when measuring 2000 AC current, which however has no impact on measuring accuracy.

(6) Current: AC+DC

Range	Resolution	Accuracy: ± (% reading + word number)
600A	0.1A	±(3.0%+20)
2500A	1A	±(5.0%+20)

Display: true RMS, applicable to 10%- 100% of the range.
Frequency response: 50Hz～60Hz
It is normal that the clamp vibrates slightly when measuring 2000 AC current, which however has no impact on measuring accuracy.

11. Current signal output function (See Figure 14)

KM 2779 clamp ammeter is provided with the current signal output function, able to convert the measured current signal into voltage signal with the ratio of 1A/1mV and output via the specific output line; by connecting output signal to measurement instrument like the oscilloscope, user can observe the wave form of current signal.

⚠ Note:

Please don't to output port input 5 V above voltage, otherwise, it will lead to instrument internal circuit damage;

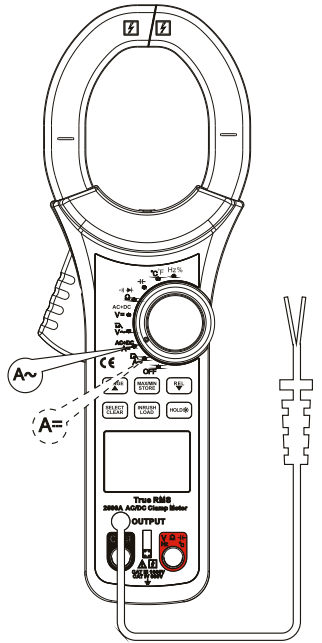


Figure 14

KUSAM-MECO®
An ISO 9001:2015 Company

12. Power gear (OFF)

Instrument should be powered off.

13. Automatic shutdown function

If not turning knob switch or pressing key on the clamp ammeter within the user-defined shutdown time (default 15min), display will be blank and enter the low power consumption dormant state. By pressing key or turn the knob switch, the instrument can be wakened up.

⚠ Note:

- Current measurement must be operated within 0℃～40℃, if positive reading is achieve after measuring DC current, the current direction will be from up to down (See Figure 10: the upward is panel and base cap is downward). Do not loosen trigger abruptly, since Hall component is sensitive in some extent to magnet, heat and mechanical stress, but also to the impact, which may cause short-time reading variation.
- Be sure the conductor to be measured is clamped at the center of clamp head, if not, an additional reading error of ±1.0% may be resulted

(7) Resistance Ω

Range	Resolution	Accuracy: ± (% reading + word number)
600Ω	0.1Ω	Under REL state: ±(1.0%+10)
6kΩ	0.001kΩ	±(0.6%+10)
60kΩ	0.01kΩ	
600kΩ	0.1kΩ	
6MΩ	0.001MΩ	±(1.2%+2)
60MΩ	0.01MΩ	±(1.5%+2)

Overload protection: 1000V

(8) Continuity test

Range	Resolution	Remark
	0.1Ω	Open-circuit voltage is about -3.5V; Sound continuity is set as <30Ω, buzzer continuously sounds. Short circuit is set as ≥30Ω, buzzer will not sound.

Overload protection: 1000V

(9) Diode

Range	Resolution	Remark
	0.001V	Open circuit voltage is about 3.5V, able to measure the PN junction ≤3V forward voltage drop value. The normal voltage value of silicon PN junction is about 0.5～0.8V.

Overload protection: 1000V

KUSAM-MECO®
An ISO 9001:2015 Company

(10) Capacitance

Range	Resolution	Accuracy: ± (% reading + word number)
60nF	0.01nF	Under REL state: ±(3%+5)
600nF	0.1nF	±(3%+5)
6μF	0.001μF	
60μF	0.01μF	
600μF	0.1μF	±(4%+5)
6000μF	1uF	±(5%+5)
60mF	0.01mF	Reference value

Overload protection: 1000V

(11) Frequency Hz

Range	Resolution	Accuracy: ± (% reading + word number)
60Hz	0.001 Hz	±(0.1%+3)
600Hz	0.01 Hz	
6kHz	0.0001kHz	
60kHz	0.001kHz	
600kHz	0.01kHz	
6MHz	0.0001MHz	
60MHz	0.001MHz	

Overload protection: 1000V
Input range a: 10Hz～40MHz: 1Vrms≤ a ≤30Vrms;
When >40MHz: unspecified.

(12) Duty ratio %

Range	Resolution	Error limit: ± (% reading + word number)
10%～90%(10Hz～2kHz)	0.01	±(1.2%+30)

Overload protection: 1000V

(13) Temperature

Range	Resolution	Error limit: ± (% reading + word number)
-40℃～40℃	1℃	±(2%+10)
40℃～400℃		±(1%+10)
400～1000℃		±2.5%
-40℉～104℉	2℉	±(2%+18)
104℉～752℉		±(1%+18)
752～1832℉		±2.5%

Overload protection: 1000V

Temperature sensor: K type (Ni-Cr and Ni- Si) thermocouple

(14) AC voltage + LPF

Range	Resolution	Remark
6V	0.001V	Intercept AC voltage signal higher than 1 KHZ
60V	0.01V	
600V	0.1V	
1000V	1V	

KUSAM-MECO®
An ISO 9001:2015 Company

(15) AC Current + LPF

Range	Resolution	Remark
600A	0.1A	Intercept AC voltage signal higher than 1 KHZ
2500A	1A	

X. MAINTENANCE AND UPKEEP

1. General maintenance

Warning: to prevent electric shocking, it is required to keep the test pen away prior to opening the base cap.

a. The clamp ammeter should be maintained and serviced by qualified professional serviceman or designated maintenance department.

b. Clean the outer case with cloth, it is forbidden to clean with cleaning agent containing abrasive material or solvent.

2. Installation or replacement of battery


6LF22 9V battery, see Figure 14, will provide power for the clamp ammeter. Please install or replace battery as follows:

a. Shut down the clamp ammeter, move away the test pen located at the input terminal.

b. Put the panel facing down, screw out the battery box screws, take off battery cap and take out battery, install new battery as per the indication of polarity.

c. It is required to install batteries of the same model. Do not install the improper battery.

D. After installing new battery, load the battery cap and screw on screws.

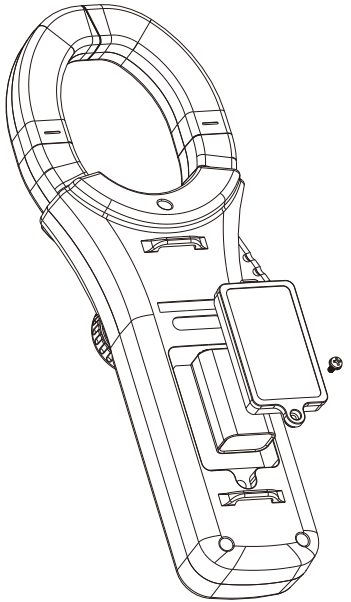

KUSAM-MECO®
An ISO 9001:2015 Company

TEST CERTIFICATE

2500A TRMS DIGITAL CLAMPMETER

This Test Certificate warrantees that the product has been inspected and tested in accordance with the published specifications.

The instrument has been calibrated by using equipment which has already been calibrated to standards traceable to national standards.

MODEL NO. _____ SERIAL NO. _____

DATE: _____

MUMBAI

ISO 9001:2015

QC
KUSAM-MECO
PASS

WARRANTY

Each “KUSAM-MECO” product is warranted to be free from defects in material & workmanship under normal use & service. The warranty period is one year (12 months) and begins from the date of despatch of goods. In case any defect occurs in functioning of the instrument, under proper use, within the warranty period, the same will be rectified by us free of charges, provided the to and fro freight charges are borne by you.

This warranty extends only to the original buyer or end-user customer of a “KUSAM-MECO” authorized dealer.

This warranty does not apply for damaged Ic’s, fuses, burnt PCB's, disposable batteries, carrying case, test leads, or to any product which in “KUSAM-MECO’s” opinion, has been misused, altered, neglected, contaminated or damaged by accident or abnormal conditions of operation or handling.

“KUSAM-MECO” authorized dealer shall extend this warranty on new and unused products to end-user customers only but have no authority to extend a greater or different warranty on behalf of “KUSAM-MECO”.

“KUSAM-MECO’s” warranty obligation is limited, at option, free of charge repair, or replacement of a defective product which is returned to a “KUSAM-MECO” authorized service center within the warranty period.

THIS WARRANTY IS BUYER’S SOLE AND EXCLUSIVE REMEDY & IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.“KUSAM-MECO” SHALL NOT BE LIABLE FOR ANY SPECIAL, INDIRECT, INCIDENTAL OR CONSEQUENTIAL DAMAGES ORLOSSES, INCLUDING LOSS OF DATA, ARISING FROM ANY CAUSE WHATSOEVER.

All transaction are subject to Mumbai Jurisdiction.

KUSAM-MECO®
An ISO 9001:2015 Company

KUSAM-MECO®

OFFICE ADDRESS SERVICE CENTER

Shop no.18, 1st Floor, CIDCO Shopping Complex, Plot # 9, Sector-7,

Rajiv Gandhi Marg, Sanpada, Navi Mumbai - 400705.

Sales Direct : +91-9867488006, 9867675093

Email : sales@kusam-meco.co.in; service@kusam-meco.co.in

Website : www.kusamelectrical.com